

NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: Guangzhou Powecom Labor Insurance Supplies Co., Ltd.

Model Tested: Powecom KN95 Protective Mask

Date Tested: May 19, 2020

These findings pertain to the Guangzhou Powecom Labor Insurance Supplies Co., Ltd., Powecom KN95 Protective Mask. The packaging and labeling for this product indicates that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator).

Ten respirators were submitted for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found [here](#).

No certificate of approval was provided with the samples received; therefore, the authenticity of the claims cannot be validated.

The maximum and minimum filter efficiency was 98.91% and 98.60%, respectively. All ten respirators measured more than 95%.

While the above-listed product classification has similar performance requirements to NIOSH-approved devices, NIOSH does not have knowledge about the sustained manufacturer quality system and product quality control for these products. NIOSH also does not have knowledge about the product's handling and exposures after leaving its manufacturer's control.

In addition, this product is an ear loop design. Currently, there are no NIOSH-approved products with ear loops; NIOSH-approved N95s have head bands. Furthermore, limited assessment of ear loop designs, indicate difficulty achieving a proper fit. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process. This assessment was developed as an assessment of the filter efficiency for those respirator's represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for [Crisis Capacity Strategies \(during known shortages\)](#).

Evaluation of International Respirators

Test: Modified TEB-APR-STP-0059

Date Tested: May 19, 2020

Report Prepared: May 20, 2020

Manufacturer: Guangzhou Powecom Labor Insurance Supplies Co., Ltd.

Item Tested: Powecom KN95 Protective Mask


Country of Certification: China (GB2626-2006)

Pictures have been added to the end of this report.

Filter	Flow Rate (Lpm)	Initial Filter Resistance (mmH ₂ O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency
1	85	10.8	1.17	1.17	98.83
2	85	10.3	1.17	1.17	98.83
3	85	11.5	1.14	1.14	98.86
4	85	10.2	1.21	1.21	98.79
5	85	10.8	1.23	1.23	98.77
6	85	11.1	1.40	1.40	98.60
7	85	10.9	1.13	1.13	98.87
8	85	11.0	1.20	1.20	98.80
9	85	11.5	1.25	1.25	98.75
10	85	11.3	1.09	1.09	98.91
Minimum Filter Efficiency: 98.60			Maximum Filter Efficiency: 98.91		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment

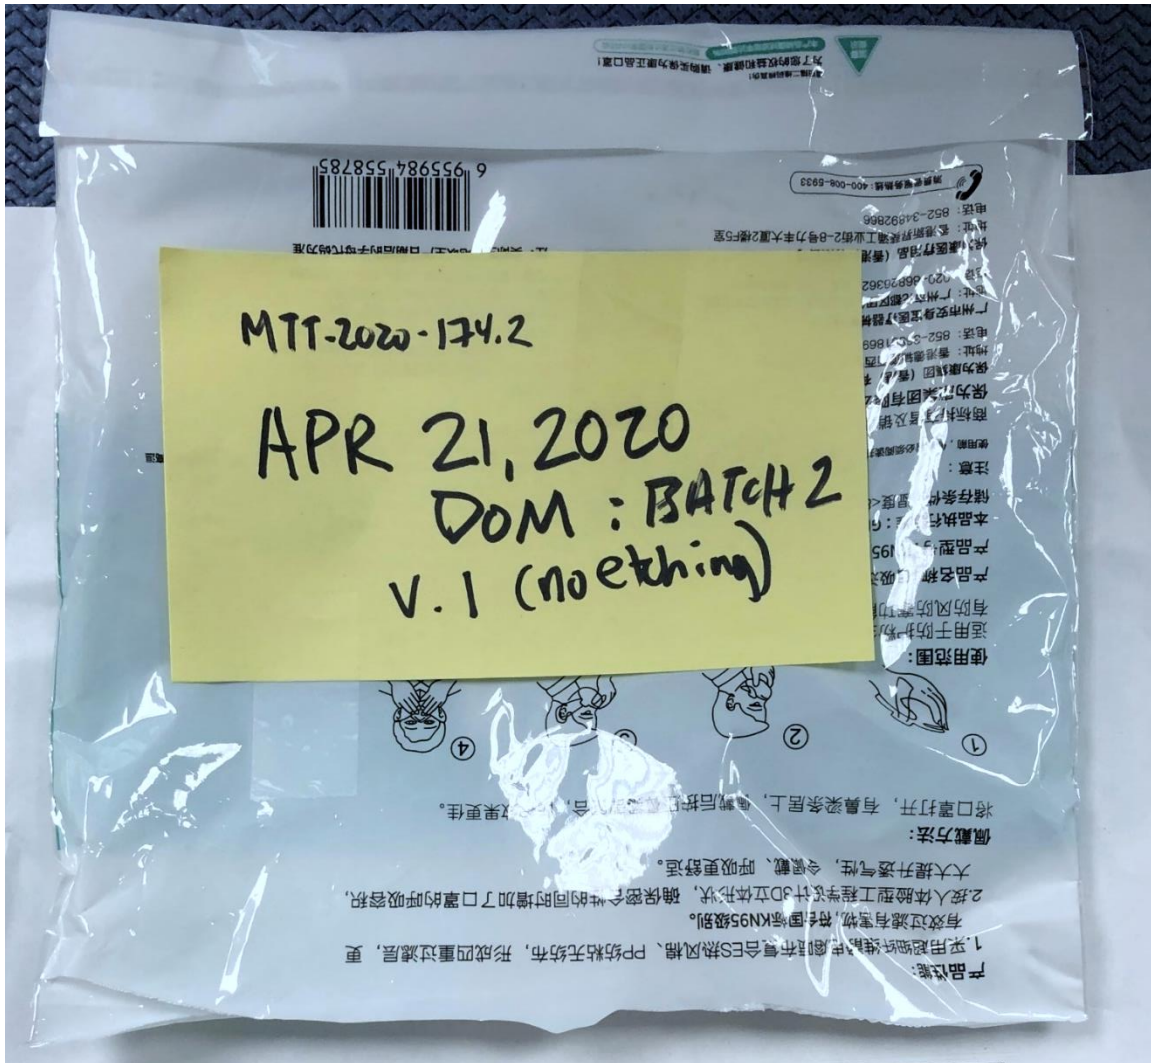



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

产品性能:
1.采用超细纤维静电喷布复合ES热风棉、PP纺粘无纺布,形成四重过滤层,更有效过滤有害物,符合国标KN95级别。
2.按人体脸型工程学设计3D立体形状,确保密合性的同时增加了口罩的呼吸容量,大幅提升透气性,令佩戴、呼吸更舒适。

佩戴方法:
将口罩打开,有鼻梁条居上,佩戴后按压鼻梁部密合,防护效果更佳。

①  ②  ③  ④ 

使用范围:
适用于防护粉尘、PM2.5雾霾颗粒物、流感细菌、飞沫等有害颗粒物。本品具有防风防寒功能。

产品名称:自吸过滤式防颗粒物呼吸器(随弃式)
产品型号:KN95 **有效期:**3年 **生产日期:**见合格证
本品执行标准:GB2626-2006 KN95
储存条件:湿度<80%,无腐蚀性气体和通风良好的清洁室内

注意:
使用前,佩戴者必须阅读并了解这些使用说明,请保存这些使用说明以便参考。

商标持有者及销售方:
保为康集团有限公司:
保为康集团(香港)有限公司
地址:香港德辅道西西营盘正街18号启正中心12楼3A
电话:852-36891869
广州市安身宝医疗器械有限公司
地址:广州市花都区团结路12号之二栋401(空港花都)
电话:020-86826362 传真:020-86600977
保为康医疗用品(香港)有限公司
地址:香港新界葵涌工业街2-8号力丰大厦2楼F5室
电话:852-34892866

注意事项:
1.为保证口罩卫生干净,要避免用手触摸接触口罩内面
2.每次佩戴防尘口罩前,应立即做佩戴“紧密性”检查,确保口罩佩戴位置正确
3.每次佩戴防尘口罩前,应该清洗双手。如需继续在粉尘多的污染环境,应该一直佩戴口罩
4.当感觉呼吸阻力明显增大,或当口罩变得脏污、破损时,应当尽快更换口罩
5.本口罩不可水洗。水洗会破坏材料结构,造成穿透。并且破坏静电滤材的过滤性能
6.未使用的口罩应储存在洁净的环境中,需防止口罩受到损坏、脏污、粘尘、阳光直射、高温或者有害化学物质污染等。存放口罩时,还要避免口罩变形。
7.口罩不能用微波炉消毒

生产方:
广州市保为康劳保用品有限公司(A)
地址:广州市花都区新雅街团结路43号保为康工业园
电话:020-86600663 传真:020-36092323
广州市白云区人和天地劳保用品厂(B)
地址:广州市白云区人和镇太成东路1号
电话:020-36092189 传真:020-36092189
注:实际生产地以生产日期后的字母代码为准

消费者服务热线:400-008-5993


6 955984 558785

请扫二维码真告!
为了您的权益和健康,请购买保为康正品口罩!

NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

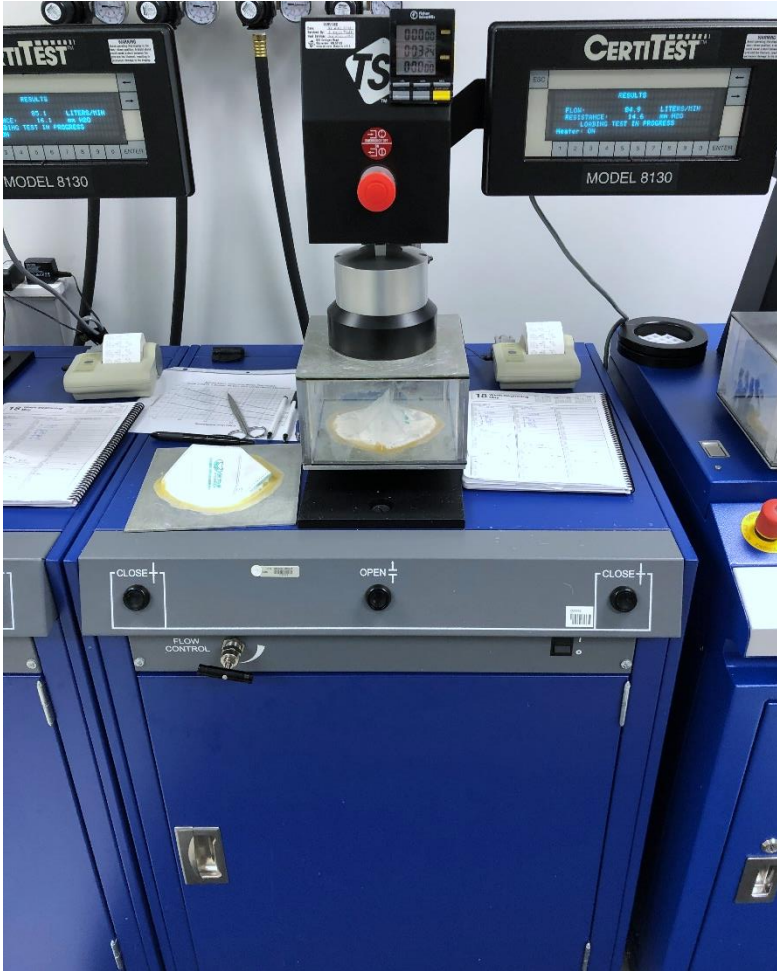

NPPTL COVID-19 Response: International Respirator Assessment

